Tristel DUO OPH™


HIGH-LEVEL DISINFECTION FOR REUSABLE TONOMETER PRISMS

NOTES

- Do not use if the bottle is damaged.
- Disinfect hands and wear suitable gloves and Personal Protective Equipment (PPE) when handling disinfectants and medical devices.
- When Tristel DUO OPH is being used for the first time, depress the pump two to four times to prime it.
- If the surface is visibly soiled, follow the hospital protocol for cleaning instructions.
- For healthcare professional use only.
- This wall chart should be used in conjunction with the instructions for use (IFU), product label, Safety Data Sheet (SDS) and device manufacturer's instructions.


DIRECTIONS FOR USE

1

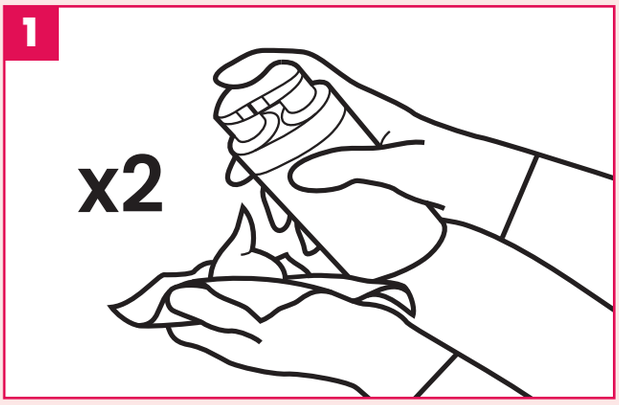

Dispense two aliquots of Tristel DUO OPH onto a dry wipe (DUO WIPES are recommended) or directly onto the tonometer prism.

2

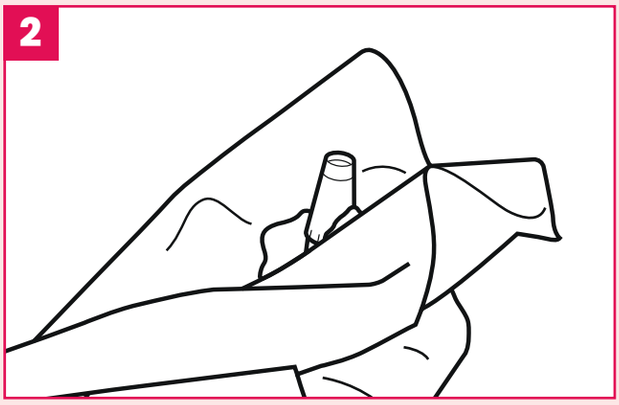

Use the wipe to spread the foam over the surface of the tonometer prism and ensure all areas are covered.


Note: Discard the used wipe and gloves in accordance with local regulations. Do not macerate. Do not reuse.

3




Leave the surface to dry to ensure a minimum contact time of 2 minutes.

4a



4b

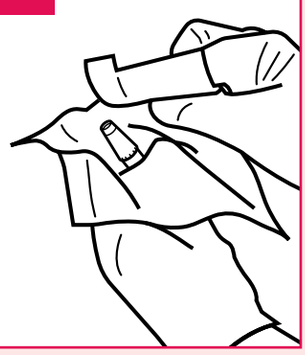

Rinse the disinfected areas with water of appropriate quality. Alternatively, pull one Tristel dry wipe out of the tub and close the cap tightly. Wipe the device once over to remove residues and dry it. Pay close attention to indentations and joins along the device.

Note: If rinsing, dry and store the medical device in accordance with hospital protocols to prevent damage or recontamination.

For Tristel patent information please visit: http://www.our-patents.info/tristel

Copyright © Tristel Solutions Limited
TRI-DUO-894a-1
18/NOV/2026

Tristel™

Tristel Solutions Limited, Unit 1b, Lynx Business Park, Fordham Road, Snailwell, Cambridgeshire, CB8 7NY, UK
T +44 (0) 1638 721500 **E** mail@tristel.com **W** www.tristel.com

Australia, Tristel Pty Ltd, Unit 44, 328 Reserve Road, Cheltenham, VIC 3192
T 1300 680 898 **E** mail-au@tristel.com **W** www.tristel.com/au-en/