Tristel Duo™ OPH



FOR REUSABLE TONOMETER PRISMS

High-level disinfectant foam

Notes:

- For professional use only.
- This wall chart should be used in conjunction with the instructions for use (IFU), product label, Safety Data Sheet (SDS) and device manufacturer's instructions.
- Disinfect hands and wear appropriate Personal Protective Equipment (PPE) when handling disinfectants and medical devices.
- Always use Tristel Duo OPH on a cleaned device.
- Follow the device manufacturer's labelling and instructions for procedures on disassembly, handling, cleaning, disinfection and rinsing.
- Do not use Tristel Duo OPH if the bottle is damaged, for longer than the prescribed contact time, or on non-compatible devices.
- If Tristel Duo OPH is used for the first time, refer to the instructions in the IFU for opening and setting up the Duo OPH bottle.
- Tristel Duo OPH efficacy may be compromised if it is used with wipes other than Duo Wipes, and if the IFU is not followed in full.

STEP 1

Dispense 3 aliquots of Tristel Duo OPH onto a Duo Wipe or directly onto the prism.

STEP 2

Use the wipe to spread the foam over the surface of the prism and ensure all areas are covered. Continuous wiping of the surface is not necessary and should be avoided to prevent shedding of the wipe.

Note: Discard the used wipe in accordance with local regulations. Do not macerate. Do not re-use.

STEP 3

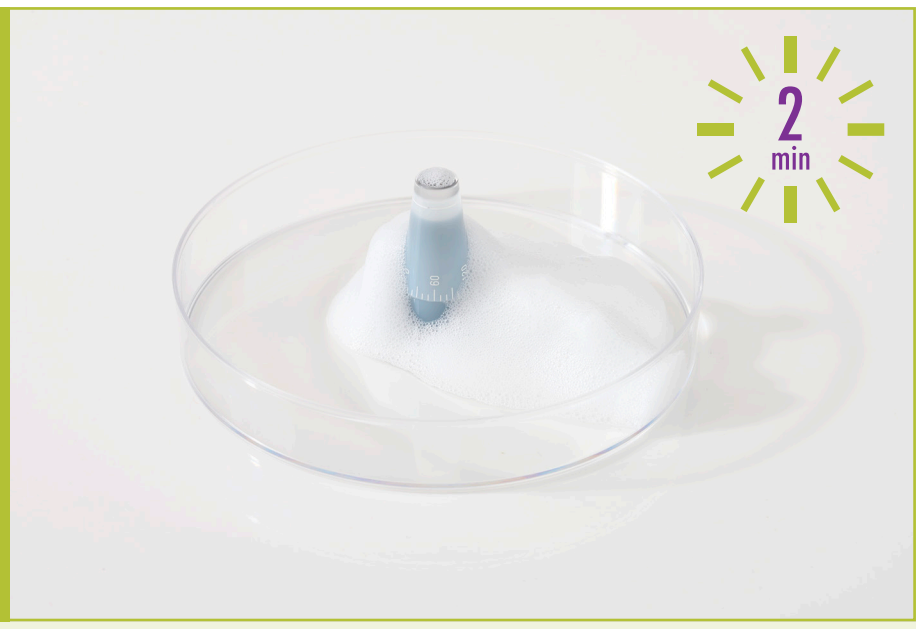

Ensure a contact time of **2 minutes**.

Note: It is recommended that a timer is used to ensure the contact time of 2 minutes is observed.

STEP 4

Rinse the prism by wiping with a Tristel Rinse Wipe or immersing it completely in sterile water. One rinse is required to remove Tristel Duo OPH residues unless more rinse cycles are specified by the device manufacturer.
Thoroughly dry all surfaces of the device using a clean soft, lint-free wipe or cloth.

Tristel™
Medical Device Decontamination

Created by: Tristel Solutions Limited, Lynx Business Park, Cambs, UK, CB8 7NY
T +44 (0) 1638 721500 - E mail@tristel.com - W www.tristel.com

Distributed by: INNOVA Medical Ophthalmics/Toronto Office, 136 Sparks Ave, Toronto ON M2H 2S4
T 416.615.0185 - E info@innovamed.com - W www.innovamed.com

For Tristel patent information please visit: http://www.our-patents.info/tristel

Copyright © Tristel Solutions
Mkt-Wal-2029-1
12/SEP/2022

Tristel™
WE HAVE CHEMISTRY.